


# 29G SPOTLIGHT DIRECTIONAL CHANDELIER


Patent Pending

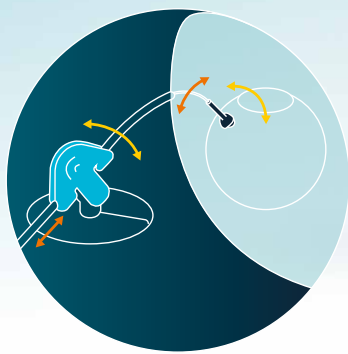

**Directional function**

**“A bright vision  
on illumination”**

Vitreco a company of:



**BVI**




**Vitreco**

# 29G Spotlight Directional Chandelier

A new generation chandelier with major improvements in functionality and ease of use.

Patent Pending

The Vitreo 29G Spotlight Directional Chandelier featuring high-end specifications with consistent performance for bimanual ophthalmic endo-illumination procedures.

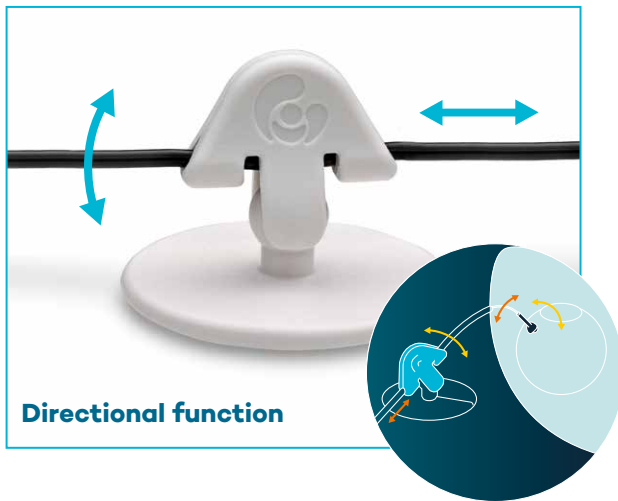

**Directional function**




“The Spotlight Directional Chandelier offers an easy and quick insertion in combination with an effective directional control of the light beam.”

Developed in collaboration with Professor Claus Eckardt

## Benefits

- Improved illumination / visualization due to directional illumination system.
- Directional Chandelier facilitates bimanual surgery.
- Adapters provide compatibility to most endo-illumination systems.

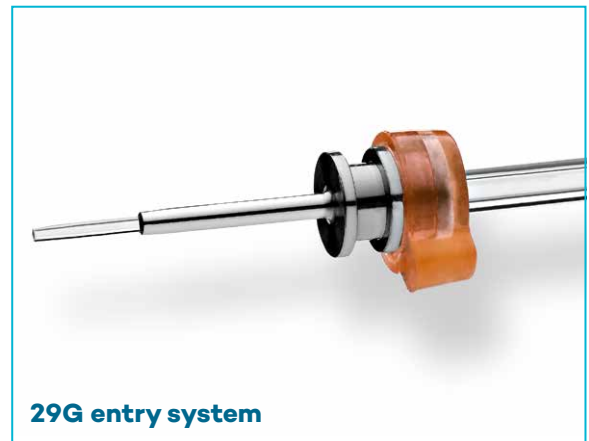

**29G entry system**



**29G minimally invasive incision**

## Features

- Directional Chandelier system designed to enhance illumination control.
- Wide view fiber tip for global endo-illumination.
- Easy insertion and fixation of the fiber with 29G valved entry system.
- 29G minimal invasive incision.
- Integrated scleral marker




## 29G Spotlight Directional Chandelier

Art.No.: LF29.D02  
Packaged box/5, Sterile




## Light Source Adaptors

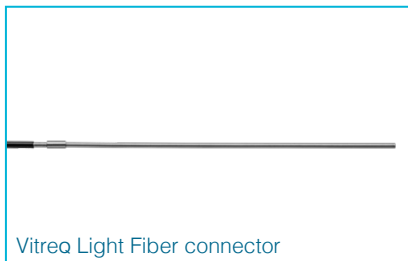

The Vitreo 29G Spotlight Directional Chandelier is compatible with most endo-illumination systems in combination with Light Source Adaptors:

- Constellation® Light Source Adaptors
- Stellaris® Light Source Adaptors
- Geuder® Light Source Adaptors
- Ruck® Light Source Adaptors
- DORC® Light Source Adaptors

|   |   |  |
|---|---|--|
| <p>Art.No.: LF00.R01</p>  <p>Constellation® Light Source Adaptor</p> | <p>Art.No.: LF00.R02</p>  <p>Stellaris® Light Source Adaptor</p> | <p>Art.No.: LF00.R03</p>  <p>Geuder® Light Source Adaptor</p> |
| <p>Art.No.: LF00.R04</p>  <p>Ruck® Light Source Adaptor</p>          | <p>Art.No.: LF00.R05</p>  <p>DORC® Light Source Adaptor</p>      |  |

\*All product names, trademarks and registered trademarks are property of their respective owners.

### Endo-Illumination Brief Statement for Vitreo Spotlight Directional Chandelier:

**Indications for Use:** Vitreo Spotlight Chandelier is intended for endo-illumination during ophthalmic surgery.

**Precautions:** Do not use product if package integrity has been breached or compromised; do not use product after the expiration date.

**Caution (USA):** Federal law restricts this device to sale by or on order of a licensed physician.

**Attention:** See Instructions for Use included in product packaging for complete listing of indications and warnings.





### ISO Certification

Vitre<sup>q</sup>'s quality system complies with the international quality and regulatory requirements and is certified by the Notified Body DQS Medizinprodukte GmbH, according to international standard ISO 13485 Medical devices – Quality management systems – Requirements for regulatory purposes.

### CE Certification

The Vitre<sup>q</sup> medical devices are certified according to the medical device directive 93/42/EEC.

### FDA

Vitre<sup>q</sup> is an FDA registered manufacturer of medical devices.

### European Countries

To order Vitre<sup>q</sup> products in Europe contact a Customer Service Representative via e-mail, telephone or fax.

#### Beaver-Visitec International, Ltd

85B Park Drive, Milton Park  
Abingdon, Oxfordshire  
OX14 4RY, United Kingdom  
**E:** [ordersuk@bvimedical.com](mailto:ordersuk@bvimedical.com)  
**T:** 44.1865.601.256 *Option 3*  
**F:** 44.1865.595.761

#### Belgium

**E:** [bestellingen@bvimedical.com](mailto:bestellingen@bvimedical.com)  
**T:** 32.52.280518 *Option 3*  
**F:** 32.52.890243

#### France, Luxembourg

**E:** [commandes@bvimedical.com](mailto:commandes@bvimedical.com)  
**T:** 33.4.85880033 *Option 3*  
**F:** 33.4.88714057

#### Germany, Switzerland, Austria

**E:** [bestellingen@bvimedical.com](mailto:bestellingen@bvimedical.com)  
**T:** 49.622.16479854 *Option 3*  
**F:** 49.622.13929883

#### Italy

**E:** [ordini@bvimedical.com](mailto:ordini@bvimedical.com)  
**T:** 39.02.89877520 *Option 3*  
**F:** 39.02.44386868

#### Netherlands

**E:** [bestellingen@bvimedical.com](mailto:bestellingen@bvimedical.com)  
**T:** 31.20808.3202 *Option 3*  
**F:** 31.20203.1293

#### Spain

**E:** [ordenes@bvimedical.com](mailto:ordenes@bvimedical.com)  
**T:** 34.91.1230335 *Option 3*  
**F:** 34.91.1849957

#### United Kingdom, Eire

**E:** [ordersuk@bvimedical.com](mailto:ordersuk@bvimedical.com)  
**T:** 44.1865.601.256 *Option 3*  
**F:** 44.1865.595.761

### North and South America

Ordering Vitre<sup>q</sup> products is easy. Contact a Customer Service Representative via e-mail, telephone or fax.

#### Beaver-Visitec International, Inc.

500 Totten Pond Rd – 10 CityPoint  
Waltham, MA 02451 USA

#### United States, Canada

**E:** [customersupport@bvimedical.com](mailto:customersupport@bvimedical.com)  
**T:** 1.866.906.8080 *Toll-free*  
781.906.8080 *Direct*  
**F:** 1.866.906.4304

#### Latin America, all other

**E:** [customersupport\\_lam@bvimedical.com](mailto:customersupport_lam@bvimedical.com)  
**T:** 781.906.8080 *Ext. 7*  
**F:** 781.906.4304

#### Japan

**E:** [bvi.cs@bvimedical.com](mailto:bvi.cs@bvimedical.com)  
**T:** 03.5651.2860  
**F:** 03.3662.2242

### All Other Regions

**E:** [ordersrow@bvimedical.com](mailto:ordersrow@bvimedical.com)  
**T:** 44.1865.601.256 *Option 3*  
**F:** 44.1865.595.761

### Vitre<sup>q</sup> Headquarters

Seggelant-Noord 2  
3237 MG Vierpolders  
The Netherlands  
**E:** [info@vitreq.com](mailto:info@vitreq.com)  
**T:** 31.181.745090  
**F:** 31.181.478583



Vitre<sup>q</sup> a company of:



[vitreq.com](http://vitreq.com) [bvimedical.com](http://bvimedical.com)

Authorized Vitre<sup>q</sup> distributor:

